

Petroleum and Liquid Petroleum Products—Calibration of Horizontal Cylindrical Tanks

Part 1: Manual Methods

ANSI/API MPMS CHAPTER 2.2E
FIRST EDITION, APRIL 2004

REAFFIRMED, AUGUST 2014

ERRATA, NOVEMBER 2009

ISO 12917-1: 2002 (identical), Petroleum and liquid petroleum products—Calibration of horizontal cylindrical tanks—Part 1: Manual methods



AMERICAN PETROLEUM INSTITUTE



Date of Issue: November 11, 2009

Affected Publication: API MPMS Chapter 2.2E, *Petroleum and Liquid Petroleum Products—Calibration of Horizontal Cylindrical Tanks, Part 1: Manual Methods*, First Edition, April 2004

ERRATA

Page 8, Clause 15

At the end of the first sentence, replace “can be neglected” with “can be neglected if H/D is less than 0,012”. At the end of the paragraph, replace “normative annex A” with “Annex A”.

Page 14, Figure A.1:

Replace items 1 and 2 in the key with the following:

Key

Value of H/D : 0,5 to 0,999 — subtract volume correction when the tank is more than half full

Value of H/D : 0,001 to 0,5 — add volume correction when the tank is less than half full

Special Notes

API publications necessarily address problems of a general nature. With respect to particular circumstances, local, state, and federal laws and regulations should be reviewed.

API is not undertaking to meet the duties of employers, manufacturers, or suppliers to warn and properly train and equip their employees, and others exposed, concerning health and safety risks and precautions, nor undertaking their obligations under local, state, or federal laws.

Information concerning safety and health risks and proper precautions with respect to particular materials and conditions should be obtained from the employer, the manufacturer or supplier of that material, or the material safety data sheet.

Nothing contained in any API publication is to be construed as granting any right, by implication or otherwise, for the manufacture, sale, or use of any method, apparatus, or product covered by letters patent. Neither should anything contained in the publication be construed as insuring anyone against liability for infringement of letters patent.

Generally, API standards are reviewed and revised, reaffirmed, or withdrawn, at least every five years. Sometimes a one-time extension of up to two years will be added to this review cycle. This publication will no longer be in effect five years after its publication date as an operative API standard or, where an extension has been granted, upon republication. Status of the publication can be ascertained from the API Standards department, telephone (202) 682-8000. A catalog of API publications, programs and services is published annually and updated biannually by API, and available through Global Engineering Documents, 15 Inverness Way East, M/S C303B, Englewood, CO 80112-5776.

This document was produced under API standardization procedures that ensure appropriate notification and participation in the developmental process and is designated as an API standard. Questions concerning the interpretation of the content of this standard or comments and questions concerning the procedures under which this standard was developed should be directed in writing to the Director of the Standards department, American Petroleum Institute, 1220 L Street, N.W., Washington, D.C. 20005. Requests for permission to reproduce or translate all or any part of the material published herein should be addressed to the Director, Business Services.

API standards are published to facilitate the broad availability of proven, sound engineering and operating practices. These standards are not intended to obviate the need for applying sound engineering judgment regarding when and where these standards should be utilized. The formulation and publication of API standards is not intended in any way to inhibit anyone from using any other practices.

Any manufacturer marking equipment or materials in conformance with the marking requirements of an API standard is solely responsible for complying with all the applicable requirements of that standard. API does not represent, warrant, or guarantee that such products do in fact conform to the applicable API standard.

All rights reserved. No part of this work may be reproduced, stored in a retrieval system, or transmitted by any means, electronic, mechanical, photocopying, recording, or otherwise, without prior written permission from the publisher. Contact the Publisher, API Publishing Services, 1220 L Street, N.W., Washington, D.C. 20005.

Copyright © 2004 American Petroleum Institute

API Foreword

API publications may be used by anyone desiring to do so. Every effort has been made by the Institute to assure the accuracy and reliability of the data contained in them; however, the Institute makes no representation, warranty, or guarantee in connection with this publication and hereby expressly disclaims any liability or responsibility for loss or damage resulting from its use or for the violation of any federal, state, or municipal regulation with which this publication may conflict.

Suggested revisions are invited and should be submitted to API, Standards department, 1220 L Street, NW, Washington, DC 20005, standards@api.org.

Currently in preview, click buy full version

Contents

	Page
API Foreword	ii
Foreword	iv
Introduction	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Precautions	2
4.1 General	2
4.2 Internal method	2
4.3 External method	2
5 Equipment	2
5.1 Equipment as used in the ISO 7507 series	2
5.2 Telescopic rod	2
6 General requirements	2
7 Calibration procedures	3
8 External measurements	3
8.1 Introduction	3
8.2 General	3
8.3 Repetition of measurements	4
8.4 Tolerances	4
8.5 Other measurements on tank-shell plates	4
9 Internal measurements	5
9.1 General	5
9.2 Repetition of measurements	5
9.3 Tolerances	5
9.4 Other measurements on tank-shell plates	5
10 Additional measurements	6
10.1 Deadwood	6
10.2 Measurement of tilt	6
11 Other parameters	7
12 Recalibration	7
13 Descriptive data	7
14 Computation of tank capacity tables — General rules	7
15 Effects of tilt	8
16 Systematic calculations (summary)	8
16.1 General	8
16.2 Cylindrical volume	8
16.3 Volume of the knuckle-dish ends	9
16.4 Elliptical ends	11
16.5 Spherical head	11
16.6 Deadwood	12
Annex A (normative) Tilt	13
Annex B (informative) Corrections of volume of tank table	15
Bibliography	18

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this part of ISO 12917 may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 12917-1 was prepared by Technical Committee ISO/TC 28, Petroleum products and lubricants, Subcommittee SC 3, Static petroleum measurement.

ISO 12917 consists of the following parts, under the general title Petroleum and liquid petroleum products — Calibration of horizontal cylindrical tanks:

- *Part 1: Manual methods*
- *Part 2: Internal electro-optical distance-ranging method*

Annex A forms a normative part of this part of ISO 12917. Annex B is for information only.

This corrected version of ISO 12917-1:2002 incorporates the following corrections.

On the cover page, “Première édition” has been replaced by “First edition”.

The missing Greek symbols have been added in the following equations:

- page 9, subclause 16.3, four equations;
- page 10, subclause 16.3, equation immediately above Figure 4;
- pages 15 and 16, clause 3.2, six equations.

Introduction

This International Standard forms part of a series on tank calibration methods. In countries where some or all of the items covered by this part of ISO 12917 are subject to mandatory regulations, the regulations have to be observed. In cases where differences exist between this part of ISO 12917 and regulations, precedence is given to the latter.

Currently in preview, click buy full version

Currently in preview, click buy full version

Petroleum and liquid petroleum products — Calibration of horizontal cylindrical tanks —

Part 1: Manual methods

1 Scope

This part of ISO 12917 specifies manual methods for the calibration of nominally horizontal cylindrical tanks, installed at a fixed location. It is applicable to horizontal tanks up to 4 m in diameter and 30 m in length.

The methods are applicable to insulated and non-insulated tanks, either when they are above-ground or underground. The methods are applicable to pressurized tanks, and to both knuckle-dish-end and flat-end cylindrical tanks as well as elliptical and spherical head tanks.

This part of ISO 12917 is applicable to tanks inclined by up to 10° from the horizontal provided a correction is applied for the measured tilt.

For tanks over and above these dimensions and angle of tilt appropriate corrections for tilt and appropriate volume computations should be based on the “Coats” equation [1].

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this part of ISO 12917. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this part of ISO 12917 are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 1998 (all parts), *Petroleum industry — Terminology*

ISO 7507 (all parts), *Petroleum and liquid petroleum products — Calibration of vertical cylindrical tanks*

3 Terms and definitions

For the purposes of this part of ISO 12917, the terms and definitions given in ISO 1998, ISO 7507-1 and the following apply.

3.1 Telescopic rod

extendable tubular measuring device to measure a distance between two points

NOTE For example, to measure the internal diameter of a cylindrical tank.

4 Precautions

4.1 General

The general and safety precautions given in ISO 7507-1 shall apply to this part of ISO 12917.

4.2 Internal method

Before a tank which has been used is entered, a safe-entry certificate, issued in accordance with local or national regulations, shall be obtained. All lines entering the tank shall be disconnected and blanked. The national or local regulations regarding entry into tanks which have contained leaded fuels shall be meticulously observed.

4.3 External method

National or local regulations regarding entry to the tank area shall be observed.

5 Equipment

5.1 Equipment as used in the ISO 7507 series

The equipment required to carry out the calibration is dependent on the method to be employed. This part of ISO 12917 uses techniques and equipment described in ISO 7507-1. Equipment used in the calibration of horizontal tanks shall conform with the specifications laid down in the relevant parts of ISO 7507. All equipment shall be traceable to a reference standard.

5.2 Telescopic rod

5.2.1 In addition to the equipment mentioned in 5.1, a telescopic rod shall be used. This telescopic rod shall have a scale capable of being read to 1 mm, and shall be calibrated to within $\pm 0,5$ mm.

5.2.2 The telescopic rod shall give a repeatability of a maximum 1 mm.

6 General requirements

6.1 The tank shall be filled to its normal working capacity and working pressure at least once and allowed to stand while full for at least 24 h prior to emptying and preparing the tank for calibration.

NOTE The hydrostatic test applied to new or repaired tanks will satisfy this requirement when additional pressure tests are carried out.


6.2 The following variables shall be considered for the development of the capacity tables:

- slope/tilt;
- dead volume;
- temperature;
- pressure;
- liquid head;
- position of gauge point.

7 Calibration procedures

The calibration procedures for calibration of horizontal cylindrical tanks are described in clause 8 (external measurements) and clause 9 (internal measurements).

For both methods, measurements will be taken at around 20 % and 80 % of the width of each ring (see Figure 1).

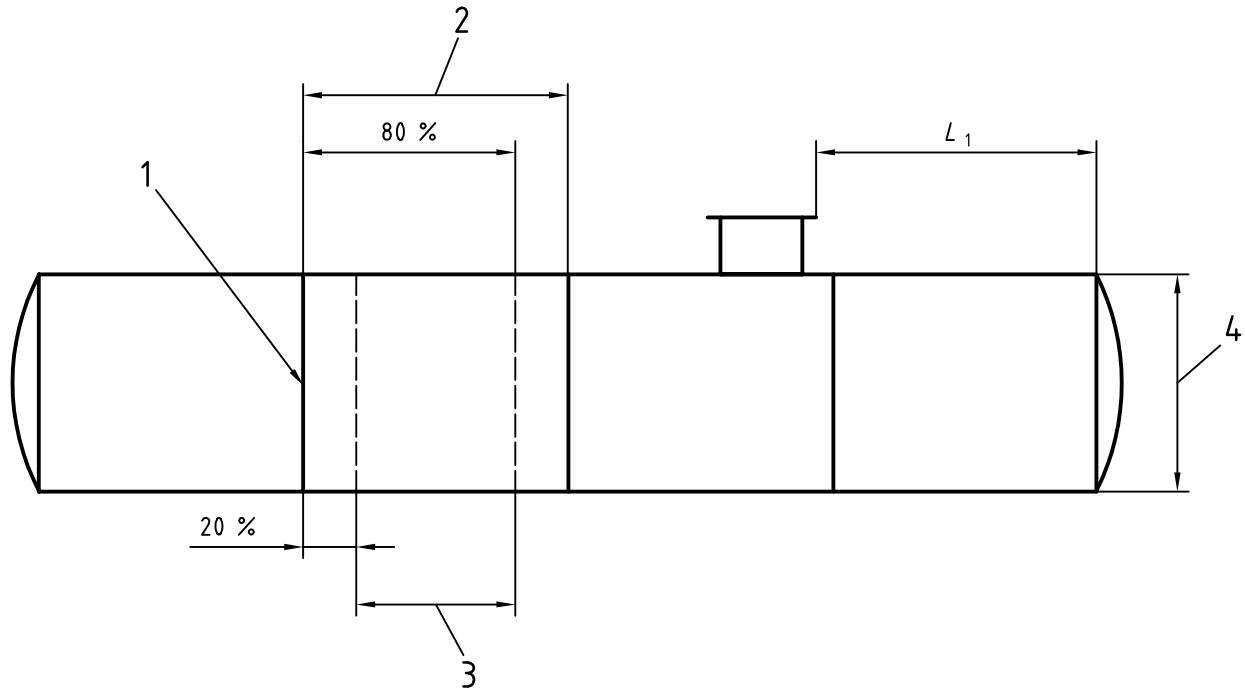

Key

- 1 Weld line
- 2 Course length
- 3 Circumference measurement
- 4 Reference height

Figure 1 — Measurements of the diameters/circumferences

8 External measurements

8.1 Introduction

External measurements may be executed with any depth of liquid and liquid pressure in the tank. The depth, temperature, density and pressure of the liquid at the time of calibration shall be recorded. However, if the temperature of the tank wall could differ by more than 10 °C between the empty part and full part of the tank whilst the measurements are being taken, the tank shall be either completely full or empty during the procedure.

8.2 General

For the measurement procedures, a circumferential tape of sufficient length to completely encircle the tank should be used and measurements of the total circumference shall be taken.

- a) In all cases, the tape to be used should be applied to the tank surface at the prescribed locations by the wraparound procedure; i.e. the required length of tape should be applied in a slack condition, positioned, and tightened by the application of the proper tension.