

ASME B89.1.17-2001

MEASUREMENT OF THREAD MEASURING WIRES

AN AMERICAN NATIONAL STANDARD



The American Society of
Mechanical Engineers

currently in preview, click buy full version



The American Society of
Mechanical Engineers

A N A M E R I C A N N A T I O N A L S T A N D A R D

MEASUREMENT OF THREAD MEASURING WIRES

ASME B89.1.17-2001

Date of Issuance: March 15, 2002

This Standard will be revised when the Society approves the issuance of a new edition. There will be no addenda issued to this edition.

ASME will issue written replies to inquiries concerning interpretations of technical aspects of this standard.

ASME is the registered trademark of The American Society of Mechanical Engineers.

This code or standard was developed under procedures accredited as meeting the criteria for American National Standards. The Standards Committee that approved the code or standard was balanced to assure that individuals from competent and concerned interests have had an opportunity to participate. The proposed code or standard was made available for public review and comment that provides an opportunity for additional public input from industry, academia, regulatory agencies, and the public-at-large.

ASME does not "approve," "rate," or "endorse" any item, construction, proprietary device, or activity.

ASME does not take any position with respect to the validity of any patent rights asserted in connection with any items mentioned in this document, and does not undertake to insure anyone utilizing a standard against liability to infringement of any applicable letters patent, nor assume any such liability. Users of a code or standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, is entirely their own responsibility.

Participation by federal agency representative(s) or person(s) affiliated with industry is not to be interpreted as government or industry endorsement of this code or standard.

ASME accepts responsibility for only those interpretations of this document issued in accordance with the established ASME procedures and policies, which precludes the issuance of interpretations by individuals.

No part of this document may be reproduced in any form,
in an electronic retrieval system or otherwise,
without the prior written permission of the publisher.

The American Society of Mechanical Engineers
Three Park Avenue, New York, NY 10016-5990

Copyright © 2002 by
THE AMERICAN SOCIETY OF MECHANICAL ENGINEERS
All Rights Reserved
Printed in U.S.A.

CONTENTS

Foreword	iv
Committee Roster	v
Committee Correspondence	vi
1 Scope	1
2 Definitions	1
3 References	1
4 General	1
5 Classification	2
5.1 Master Wires	2
5.2 Working Sets	2
6 Inch Series Specifications	2
6.1 Material	2
6.2 Wire Design	2
6.3 Wire Tolerances	2
6.4 “Best-Size” Wires	3
6.5 Wire Measurement Methods	4
7 Metric Series Specifications	5
7.1 Material	5
7.2 Wire Design	6
7.3 Wire Tolerances	6
7.4 “Best-Size” Wires	6
7.5 Wire Measurement Methods	6
Figures	
1 Threading Measuring Wires	2
2 Measuring Instrument	7
Tables	
1 “Best-Size” Wires for Inch Series 60 deg Threads	3
2 “Best-Size” Wires for Inch Series 29 deg Acme Threads	4
3 “Best-Size” Wires for Inch Series 7/45 deg Buttress Threads	4
4 Thread Wire Measurement Specifications	5
5 “Best-Size” Wires for Metric Series 60 deg Threads	7
6 Thread Wire Measurement Specifications	7
Nonmandatory Appendices	
A Measurement of Balls	9
B Examples of Uncertainty Budgets for Thread Wire Measurements	11

FOREWORD

This Standard is the result of the combined work of members of the ASME B1 Screw Thread Committee and the ASME B89 Dimensional Metrology Committee. It is the responsibility of the B1 Committee to determine how the pitch diameter of threads is measured. The B89 Dimensional Metrology Committee writes standards on specifications and procedures for dimensional measuring equipment. Thread wires differ from most wires measured in that they are measured in a deformed condition to approximate the elastic deformation that occurs when they are used to measure pitch diameter.

For this reason when using this Standard it is necessary to ensure that the B1 standards referenced in this document are the latest edition of the B1 standard which specifies the conditions to be used when measuring the pitch diameters of threads.

The measurement of thread measuring balls is included as an appendix to the standard.

This edition of B89.1.17 was approved by the American National Standards Institute on October 24, 2001.

ASME B89 STANDARDS COMMITTEE

Dimensional Metrology

(The following is the roster of the Committee at the time of approval of this Standard.)

OFFICERS

R. B. Hook, *Chair*
M. Lo, *Secretary*

COMMITTEE PERSONNEL

D. Beutel, Caterpillar, Inc.
K. L. Blaedel, University of California
J. B. Bryan, Bryan Associates
T. Carpenter, U.S. Air Force
T. Charlton, Brown and Sharpe Manufacturing
R. J. Hocken, University of North Carolina
R. B. Hook, Metcon
M. Liebers, Professional Instruments Co.
M. Lo, The American Society of Mechanical Engineers
B. Parry, Boeing Co.
F. G. Parsons, Federal Products Co.
B. R. Taylor, Renishaw PLC
R. C. Veale, National Institute of Standards and Technology (Retired)

SUBCOMMITTEE B89.1 — LFNC

R. C. Veale, *Chair*, National Institute of Standards and Technology (Retired)
D. Carlson, L. S. Starrett
D. Christy, Federal Products Co.
T. D. Doiron, National Institute of Standards and Technology
D. D. Friedel, L. S. Starrett
C. J. Fronczek, Jr., National Institute of Standards and Technology
M. R. Hamar, Professional Instruments, Inc.
D. T. Harris, Southern Gage, Inc.
G. L. Vander Sande, U.S. Army Armaments Research
W. A. Watts, Southern Gage, Inc.

WORKING GROUP B89.1.17 — MEASUREMENT OF THREAD MEASURING WIRES

R. C. Veale, *Chair*, National Institute of Standards and Technology (Retired)
A. Barrows, Kennametal
L. Dixon, Jr., General Electric
R. Dodge, Penney-Dodge
T. D. Doiron, National Institute of Standards and Technology
D. T. Harris, Southern Gage, Inc.
R. Iavelli, Deltronic Corp.
L. Johnson, Johnson Gages
J. Kane, Boeing Co.
R. Knittel, Leitech — U.S., Ltd & AMTMA

W. C. Lehmus, GagedoctRx, LLC
R. Larzelere, Deltonic Corp.
S. Ramsdale, Honeywell
P. Schmitt, R. L. Schmitt Corp.
A. G. Strang, National Institute of Standards and Technology (Retired)
P. Tuller, Mahr Federal, Inc.

Currently in preview, click buy full version

CORRESPONDENCE WITH B89 COMMITTEE

General. ASME Codes and Standards are developed and maintained with the intent to represent the consensus of concerned interests. As such, users of this Standard may interact with the Committee by requesting interpretations, proposing revisions, and attending Committee meetings. Correspondence should be addressed to:

Secretary, B89 Main Committee
The American Society of Mechanical Engineers
Three Park Avenue
New York, NY 10016

Proposing Revisions. Revisions are made periodically to the Standard to incorporate changes that appear necessary or desirable, as demonstrated by the experience gained from the application of the Standard. Approved revisions will be published periodically.

The Committee welcomes proposals for revisions to this Standard. Such proposals should be as specific as possible, citing the paragraph number(s), the proposed wording, and a detailed description of the reasons for the proposal, including any pertinent documentation.

Interpretations. Upon request, the B89 Committee will render an interpretation of any requirement of the Standard. Interpretations can only be rendered in response to a written request sent to the Secretary of the B89 Main Committee.

The request for interpretation should be clear and unambiguous. It is further recommended that the inquirer submit his/her request in the following format:

Subject: Cite the applicable paragraph number(s) and the topic of the inquiry.
Edition: Cite the applicable edition of the Standard for which the interpretation is being requested.
Question: Phrase the question as a request for an interpretation of a specific requirement suitable for general understanding and use, not as a request for approval of a proprietary design or situation. The inquirer may also include any plans or drawings which are necessary to explain the question; however, they should not contain proprietary names or information.

Requests that are not in this format will be rewritten in this format by the Committee prior to being answered, which may inadvertently change the intent of the original request.

ASME procedures provide for reconsideration of any interpretation when or if additional information that might affect an interpretation is available. Further, persons aggrieved by an interpretation may appeal to the cognizant ASME Committee or Subcommittee. ASME does not “approve,” “certify,” “rate,” or “endorse” any item, construction, proprietary device, or activity.

Attending Committee Meetings. The B89 Main Committee regularly holds meetings, which are open to the public. Persons wishing to attend any meeting should contact the Secretary of the B89 Main Committee.

Page intentionally blank

Currently in preview, click buy full version

MEASUREMENT OF THREAD MEASURING WIRES

1 SCOPE

This Standard is intended to establish uniform practices for the measurement of thread measuring wires. The standard includes methods for the direct measurement of both master and working wires, and methods for the comparison measurement of working wires. The standard includes requirements for geometric qualities of thread measuring wires, the important characteristics of the comparison equipment, environmental conditions, and the means to ensure that measurements are made with an acceptable uncertainty level.

Wires covered by the standard include inch series 60-deg, 29-deg Acme, 7/45-deg Buttress, and metric 60-deg threads.

2 DEFINITIONS

“best-size” wire: the size of a wire that would touch at the pitch cylinder on a thread of zero lead angle.

“C” constant: a constant to be subtracted from the measurement over the wires to give the pitch diameter

measurement uncertainty: parameter associated with the result of a measurement that characterizes the dispersion of the values that could reasonably be attributed to the measurand (quantity being measured).

3 REFERENCES

The following documents form a part of this Standard to the extent specified here. The latest issue shall apply.

- ASME B1.2, Gages and Gaging for Unified Inch Screw Threads
- ASME B1.5, Acme Screw Threads
- ASME B1.7M, Nomenclature, Definitions, and Letter Symbols for Screw Threads
- ASME B1.8, Stub Acme Screw Threads
- ASME B1.9, Buttress Inch Screw Threads 7°/45° Form with 0.6 Pitch Basic Height of Thread Engagement
- ASME B1.16M, Gages and Gaging for Metric M Screw Threads
- ASME B1.22M, Gages and Gaging for MJ Series Metric Screw Threads

ASME B1.30M, Screw Threads — Standard Practice for Calculating and Rounding Dimensions

Publisher: The American Society of Mechanical Engineers (ASME), Three Park Avenue, New York, NY 10016-5990; Order Department: 22 Law Drive, Box 2900, Fairfield, NJ 07007-2900

Federal Specification GGG-W-366b, Federal Specification Wire, Measuring: Gear, Thread, and General Purpose, General Services Administration, Washington, DC, May 8, 1967 (canceled)

Guide to the Expression of Uncertainty in Measurement


Publisher: International Organization for Standardization (ISO), 1 rue du Savarémé, Case Postale 56, CH-1211, Geneva, 20, Switzerland/Suisse

NIST Technical Note 1297, 1994 Edition, Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results

Puttock, M. J. and Thwaite, E. G., “Elastic Compression of Spheres and Cylinders at Point and Line Contact,” National Standards Laboratory Technical Paper No. 25, Commonwealth Scientific and Industrial Research Organization (CSIRO), Australia, 1969

4 GENERAL

When the pitch diameter of external threads is measured using thread wires, good repeatability is only obtained when a sufficient force is used to push the wires against the sides of the thread flank. Elastic deformation occurs between the wires and thread flanks when the pitch diameter is measured in this manner. The practice in the United States is to measure the wires with a method that approximately reproduces the deformation that occurs between the thread and the wires. For the thread series listed in this Standard, the ASME B1 Committee has standardized the forces to be used when measuring pitch diameter. In measuring the pitch diameter of internal threads, and in some cases external threads, balls rather than wires are used. The use of balls for measuring pitch diameter is discussed in Appendix A.

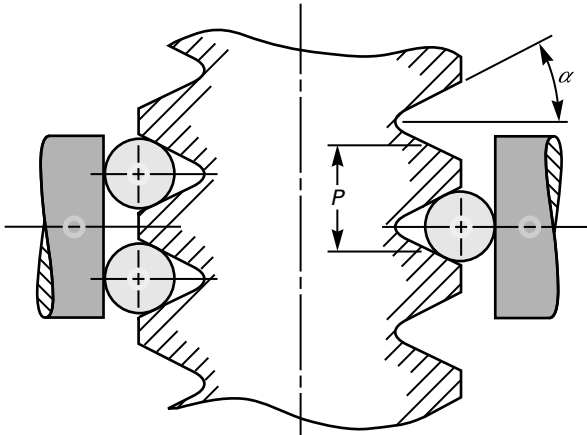

GENERAL NOTES:
 (a) P is the pitch.
 (b) α is the half-angle.

FIG. 1 THREADING MEASURING WIRES

5 CLASSIFICATION

Wires may be classified by their use as masters or working wires and by inch or metric series.

5.1 Master Wires

Master wires contain only one wire per pitch. The wires are used to measure working wires or, in some cases, other master wires.

5.2 Working Sets

Wires meant for measuring the pitch diameter of threaded gages or products consist of a three-wire set for each pitch. The wires may be measured either by comparison to a master, which has been measured in accordance with this Standard, or by directly measuring the wires in the manner described in the standard. See Fig. 1.

6 INCH SERIES SPECIFICATIONS

The material and design specifications for all master and working wires are the same, except that the working wires, which are three-wire sets, have a requirement that the variation in diameter among the three wires may not exceed a specified amount. A correction factor (“C” constant) must also be calculated and placed on the label for all except 29-deg Acme wires.

6.1 Material

The wires shall be made from alloy tool steel that has been stabilized to ensure dimensional stability. The

wires shall be free from cracks and other detrimental defects. The hardness shall be a minimum of 62 on the Rockwell C scale. The surface finish shall not exceed $2 \mu\text{in. } R_a$, using a 0.03-in. cutoff.

6.2 Wire Design

A set of measuring wires shall consist of three wires for each pitch, except for master wires, which contain one wire for each pitch. The length of the thread wires shall be a minimum of 1 in. Variations in the length of the three wires in any set shall not exceed 0.1 in.

6.3 Wire Tolerances

In order to accurately measure the pitch diameter of threaded gages and thread products, it is necessary to have accurate measurements of the wires. For example, an error of one unit in the mean diameter of thread measuring wires will cause an error of three units (for 60-deg threads) when measuring pitch diameter.

6.3.1 Master Wires. Diameters of master wires need to be known, in most cases, with an uncertainty of $5 \mu\text{in.}$ or less. The diameter of the wires shall be within $20 \mu\text{in.}$ of the “best-size” as shown in the tables or computed using the formulas in this document. The variations in diameter, including taper and out-of-roundness, shall not exceed $5 \mu\text{in.}$ over the central 0.5 in. of the wire.

6.3.2 Working Sets. A set of wires shall have the same diameter within $10 \mu\text{in.}$, and the average diameter shall be within $20 \mu\text{in.}$ of the specified “best-size” wire. The variations in diameter of each wire, including taper and out-of-roundness, shall not exceed $10 \mu\text{in.}$ over the central 1 in. of the wire. Each set shall display the TPI (threads per in.) and the average deformed diameter. Except for 29-deg Acme, the calculated wire constant (“C” constant), based on the measured mean diameter, shall also be displayed. The “C” constant for symmetrical threads is computed from the formula

$$C = w (1 + \text{cosec } \alpha) - [\cot(\alpha)/2n]$$

where

w = the average of the set

α = the half-angle, and

n = the number of threads per in.

For 60-deg threads the formula reduces to